SNAPSHOOT
ENGINEERED FOR A SAFER TOMORROW

현장을 이해하고, 필요한 솔루션을 연결합니다.

산업안전 · 추락방지 시스템
산업용 소재 · 건축자재
제품 제안부터 공급·시공·설치·교육까지



COMPANY INFORMATION

스냅슛 (SNAPSHOOT)

ADDRESS (15431) 경기도 안산시 단원구 풍전로 37-9 트리플렉스 301동 118호
TEL 0507-1374-9229
FAX 0504-481-6749
E-MAIL bkkim@snapshoot.co.kr

TECHNICAL DOCUMENTS

인증서 · 데이터시트 · 기술자료

제품의 규격과 성능, 인증 및 적용 조건을 확인하기 위한 자료입니다.

ABOUT SNAPSHOOT

제품 공급을 넘어, 현장에 맞는 해결책으로

스냅슛은 산업현장의 작업 환경과 요구 조건을 바탕으로
적합한 제품과 시스템을 제안합니다. 현장 실사를 통해 설치 조건을 확인하고,
공급부터 시공·설치 및 사용 교육까지 필요한 과정을 함께합니다.

추락방지 시스템

안전대부착설비 · 수평·수직 라이프라인
레일 시스템 · 리지드 포스트

밀폐공간 진입·구조 솔루션

데빗암 · 삼각대 · 구조용 윈치
윈치 안전블록 · 구조장비

산업안전 보호구

전신형 안전대 · 랜야드 · 안전블록
작업 환경에 맞춘 개인보호구

산업용 소재·건축자재

산업용 테이프 · 접착제 · 기능성 소재
구조용 스크류 · 목조건축 자재

SNAPSHOOT
ENGINEERED FOR A SAFER TOMORROW

홈페이지 바로가기 →
문서 라이브러리 바로가기 →
시공사례 바로가기 →
문의하기 →

본 페이지는 스냅슛의 자료 제공 안내용 표지입니다. 첨부된 인증서 및 기술자료의 발행 주체, 인증 대상과 적용 범위는 해당 원문을 기준으로 확인해 주세요.



Rapid detection from the start

Neogen® Molecular Detection Assay 2 (MDA 2) - *Cronobacter*

The first isothermal molecular method for the detection of Cronobacter spp.

Cronobacter has emerged as a pathogen of concern in Powdered Infant Formula (PIF). Producers need rapid, easy-to-use, and specific detection methods.

A simplified workflow with fewer steps and no prep helps you save time and reduce costs. Next-day results mean you can take action sooner. As part of the Neogen Molecular Detection System, you can be confident with information you can trust.

Get results. Make decisions. Take action.

Using a combination of advanced technologies — isothermal DNA amplification and bioluminescence detection — the Neogen MDA 2 - *Cronobacter* overcomes the limitations of traditional agar and PCR-based methods.

Compared to Agar

- Faster results — saves up to 2–4 days
- Simple use, fewer steps — no agar media prep
- Automated interpretation — eliminate subjective analysis of colonies

Compared to PCR


- Single, non-selective enrichment step
- Increased productivity with no reagent prep and a simplified workflow

The Neogen MDA 2 - *Cronobacter* detects the latest taxonomic classification of *Cronobacter* species with 100% inclusivity and exclusivity.


Testing Method	Cross-reaction with *Non-Cronobacter*
Commercial chromogenic agar	Cross-reaction (False Positive)[1]
Commercial PCR system	Cross-reaction (False Positive)[1]
Neogen MDA 2 - *Cronobacter*	No cross-reaction (Negative)

A family working together.

Neogen brings you a total solution with results in 24 hours.

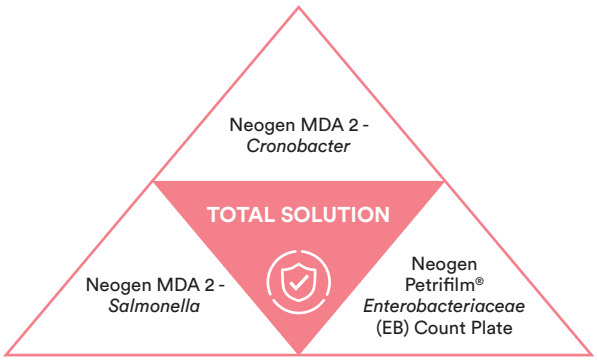


Learn more at **info.neogen.com/MDS**



Certifications and Validations:

- AOAC® *Performance Tested Method*℠ (Certificate #101703)
- AOAC *Official Method of Analysis*℠ (AOAC 2018.01)
- NF VALIDATION certificate granted by AFNOR Certification, 3M 01/20 - 03/18

Simple and Streamlined Workflow

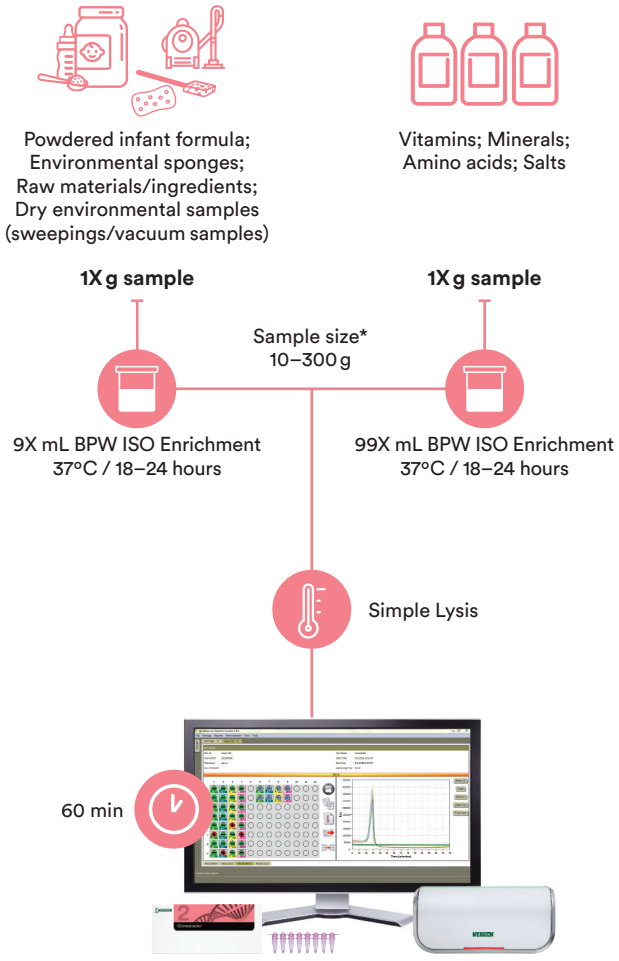

* Varies by matrix; see product instructions.

Ordering Information

Description	Cat. No.	Contents
Molecular Detection Assay 2 - *Cronobacter*	MDA2CRO96	96 tests/kit

NEOGEN

[1] 3rd party testing showed false-positive result for powdered infant formula spiked with *Siccibacter turicensis*

[2] U.S. Food & Drug Administration Bad Bug Book 2nd Edition

Neogen Corporation, 620 Lesher Place, Lansing, MI 48912 USA.

© Neogen Corporation 2023. All rights reserved. Neogen and Petrifilm are registered trademarks of Neogen Corporation.
All other marks mentioned are the property of their respective owners.

FS00034_0523